


HOSPITAL BIDS AND AWARDS COMMITTEE
SUPPLEMENTAL BID BULLETIN NO. 2
IB 2021-011B – SUPPLY & DELIVERY OF VARIOUS MEDICAL EQUIPMENT SET2
IB2021-011C – SUPPLY & DELIVERY OF VARIOUS PRINTERS
PRE-BID CONFERENCE (JULY 22, 2021)

I. GENERAL INSTRUCTIONS

- Bidders are required to submit one (1) soft copy of the original documents clearly scanned in multiple pages in one (1) PDF File per the three required files to the designated Google Form link.
- Documentary requirements on the electronic bidding is the same as in the manual bidding as provided in the 2016 Revised Implementing Rules and Regulations (IRR) of Republic Act 9184 (RA 9184), otherwise known as the “Government Procurement Reform Act” and Resolution No. 09-2020 of the Government Procurement Policy Board entitled “Approving Measures for the Efficient Conduct of Procurement Activities During a State of Calamity, or Implementation of Community Quarantine or Similar Restrictions”
- The BAC is using the 6th Edition of the Philippine Bidding Documents and all Amendments Forms therein.
- Due to limited slots in Zoom, only one (1) representative per bidder will be allowed to enter.
- Bidder shall only provide the password of their encrypted file upon being called and acknowledged in the Online Bidding Conference by the BAC before the opening of said Bidder’s bid documents. Bidder’s video should be on during this process.
- For the issuance of the Official Receipt, bidders may get the same at the Cash Collection Section or Procurement Section, during office hours, M-F; 8:00AM-5:00PM, except holidays, and upon showing of proof of payment. For the purpose of the bidding, those who submitted the proof of payment early will be verified by our Cash Collection Section and will be provided a soft copy of the Official Receipt, otherwise, other proof of payment will be acceptable subject to later verification by the Cash Collection Section.
- The winning bidder is required to produce two (2) hard copies of the scanned document anytime before the award. The same can be personally sent or via courier. Any discrepancy on the submitted soft copy as bidder during the bidding conference and hard copies as winning bidder is a ground for disqualification.
- The scanned copy should have the required original signature. E-signature is not allowed.
- Bidders must submit updated Tax clearance per E.O. No. 398, s. 2005, as finally reviewed and approved by the Bureau of Internal Revenue (BIR).
- It is understood that the Contractor is legally responsible to deliver all issued purchase order/s and failure to deliver the first Purchase Order as scheduled shall mean automatic cancellation of the PO and Notice of Award (NOA). Upon cancellation, the BAC shall proceed to qualify the second lowest bidder if applicable; or proceed to Negotiated Procurement. The Winning Contractor who failed to deliver shall shoulder the price difference (from the second lowest bidder) of the item in addition to the acquired liquidated damages.
- In lieu of the Certificate of Ongoing Projects/Accomplishments, Bidders must present their progress report or percentage of partial accomplishment, together with their contracts, awards, and proof of deliveries such as sales invoice.

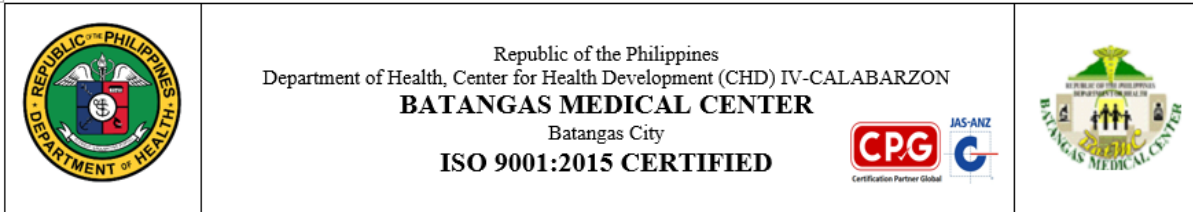

- Bidders must specify in the Technical Specifications Form under Bidder’s Offer, Technical Specifications Column the exact specifications they are offering submitted against each of the individual parameters. Whereas, bidders must state either “Comply” or “Not Comply” under the Bidder’s Offer, Statement of Compliance Column. The bids with incomplete and incorrect filled out Technical Specifications Form will be disqualified.
- Bidder must have completed, within the period specified in the Invitation to Bid, an SLCC that is similar to the contract to be bid, and whose value, adjusted to current prices using the Philippine Statistics Authority (PSA) consumer price indices, must be at least fifty percent (50%) of the ABC. However, in the case of Expendable Supplies, said SLCC must be at least twenty five percent (25%) of the ABC. Service will fall on the Expendable Supplies.
- If there is no single completed contract for the required amount, the bidder may submit at least two (2) completed similar contracts and the aggregate contract amounts should be equivalent to at least the percentage of the ABC as required above and the largest of these similar contracts must be equivalent to at least half of the percentage of the ABC as required.
- A contract shall only be considered “similar” to the contract to be bid if it is of similar nature.
- Contracts similar to the Project should be completed within two (2) years to the deadline for the submission and receipt of bids.

II. Amendment on **Section VI. Schedule of Requirements (Delivery Schedule)** as per Pre-Bidding Conference conducted last July 22, 2021 as follows:

IB2021-011B – Supply & Delivery of Various Medical Equipment Set 2





FROM	TO
30-60 CALENDAR DAYS	<i>SEE REQUIRED DELIVERY SCHEDULE UNDER THE TECHNICAL SPECIFICATION FORM OF EACH MEDICAL EQUIPMENT</i>

III. Amendments on the **Section VII. Technical Specifications** as per Pre-Bidding Conference conducted last July 22, 2021 as follows:

IB2021-011B – Supply & Delivery of Various Medical Equipment Set 2

A. Item 1: Newborn Screening Device (Otoacoustic Emission Machine)

FROM	TO
Purpose of use	Purpose of use
Newborn hearing screening test for well and sick babies as well as those admitted at the COVID-19 ward	Newborn hearing screening test for well and sick babies as well as those admitted at the COVID-19 ward
<u>Utility Requirements:</u>	<u>Utility Requirements:</u>
Power supply: Lithium-ion rechargeable battery Battery life: 500-1000 tests per charge, at least	Power supply: Lithium-ion rechargeable battery Battery life: 500-1000 tests per charge, at least

	<p>Republic of the Philippines Department of Health, Center for Health Development (CHD) IV-CALABARZON BATANGAS MEDICAL CENTER Batangas City ISO 9001:2015 CERTIFIED</p> <div style="display: flex; justify-content: space-around; align-items: center;">   </div>	
---	--	---

15 hours on- me	15 hours on-time
-----------------	------------------

B. Item 2: Low Intensity Laser

FROM	TO
<p>PHYSICAL DESCRIPTION</p> <p>Dimensions device (length 22-25 x 16-20 x 14 cm) Weight Unit: 1-3 kilograms</p>	<p>PHYSICAL DESCRIPTION</p> <p>Dimensions device (length 22-39 x 14-20 x 14 cm) Weight Unit: 1-4 kilograms</p> <p>Device should fit in the mobile cart. Mobile cart should be able to hold and carry the weight of the unit.</p>

C. Item 3: Hand Dynamometer

TO OMIT FROM THE LIST OF MEDICAL EQUIPMENT FOR PUBLIC BIDDING
--

D. Item 4: Hand Exerciser/Power Web



FROM	TO
<p><u>PHYSICAL DESCRIPTION</u></p> <p>weight: .5 – 1.5 lb. each Color coded: yellow – light resistance red – medium resistance green – heavy resistance blue – X – heavy resistance black – XX- heavy resistance</p>	<p><u>PHYSICAL DESCRIPTION</u></p> <p>weight: .5 – 2 lb. each Color coded: yellow – light resistance red – medium resistance green – heavy resistance blue – X – heavy resistance black – XX- heavy resistance not particular with the colours but should comply with the specified resistances</p>

E. Item 5: Biofeedback Machine

FROM	TO
<p><u>DELIVERY</u></p> <p>30 to 60 days from the receipt of Purchase Order</p>	<p><u>DELIVERY</u></p> <p>30 to 90 days from the receipt of Purchase Order</p>

F. Item 9: 2 Units Slit Lamp Biomicroscope with Camera

FROM	TO
<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p>	<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p>

	<p>Republic of the Philippines Department of Health, Center for Health Development (CHD) IV-CALABARZON BATANGAS MEDICAL CENTER Batangas City ISO 9001:2015 CERTIFIED</p>	
---	--	---

	<p>Requirements for sign-off: Supplier to perform installation, safety and operation checks before handover. Local clinical staff to affirm completion of installation.</p> <p>Training of staff (medical, technicians): Training of users in operation and basic maintenance shall be provided. Advanced maintenance tasks required shall be documented.</p>
<p><u>WARRANTY</u></p> <p>C. Service Unit:</p> <p>a. In case of Unit Malfunction, Bidder must provide a service unit within 48 hours until such time that the unit has been repaired or replaced.</p>	<p><u>WARRANTY</u></p> <p>C. Service Unit:</p> <p>a. In case of Unit Malfunction, Bidder must provide a service unit within 24-72 hours until such time that the unit has been repaired or replaced.</p>
<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine has been in the local or international market for at least five (5) years.</p>	<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the hospital equipment/machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that hospital equipment/machine has been in the local or international market for at least five (5) years.</p>

G. Item 10: 1 Unit Auto-refractometer with keratometer





FROM	TO
<p>Keratometer</p> <ol style="list-style-type: none"> 1. Should have (15x / 10x) eye piece 2. Should measure corneal refractive power measuring range from 36 to 52 D in steps of 0.25D steps 3. Should measure corneal radius of curvature measuring range from 5 to 10 mm in steps of 0.05mm 4. Should have high accuracy of measurements 5. Should have dust cover and spare bulb. 6. Should have well illuminated circular mires with + sign. 	<p>Keratometer</p> <p>Radius of Curvature: approx. 5.0~13.0mm (increments : 0.01mm)</p> <p>Corneal Power: approx. 25.96~67.50D (increments : 0.05, 0.12, 0.25D) (When corneal equivalent refractive index is 1.3375)</p> <p>Corneal Astigmatism: approx. 0.00~ - 15.00D (increments : 0.05, 0.12, 0.25D)</p> <p>Axis: 0~180° (increments : 1°)</p> <p>Pupil, Iris Diameter: approx. 2.0~14.0mm (increments : 0.1mm)</p>



Republic of the Philippines
 Department of Health, Center for Health Development (CHD) IV-CALABARZON
BATANGAS MEDICAL CENTER
 Batangas City
ISO 9001:2015 CERTIFIED



<p><u>PHYSICAL DESCRIPTION</u> Dimensions: Minimum 260 x 490 x 470mm Weight (lbs, kg): approx. 15kg-19kg</p>	<p><u>PHYSICAL DESCRIPTION</u> Dimensions: Minimum 260 x 490 x 457mm Weight (lbs, kg): approx. 15kg-20kg</p>
<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p>	<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p> <p>Requirements for sign-off: Supplier to perform installation, safety and operation checks before handover. Local clinical staff to affirm completion of installation.</p> <p>Training of staff (medical, technicians): Training of users in operation and basic maintenance shall be provided. Advanced maintenance tasks required shall be documented.</p>
<p><u>WARRANTY</u></p> <p>C. Service Unit:</p> <ol style="list-style-type: none"> a. In case of Unit Malfunction, Bidder must provide a service unit within 48 hours until such time that the unit has been repaired or replaced. 	<p><u>WARRANTY</u></p> <p>C. Service Unit:</p> <ol style="list-style-type: none"> a. In case of Unit Malfunction, Bidder must provide a service unit within 24-72 hours until such time that the unit has been repaired or replaced.
<p><u>DOCUMENTATION</u></p> <ol style="list-style-type: none"> a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine has been in the local or international market for at least five (5) years. 	<p><u>DOCUMENTATION</u></p> <ol style="list-style-type: none"> a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the hospital equipment/machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery . c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that hospital equipment/machine has been in the local or international market for at least five (5) years.
<p><u>DOCUMENTATION</u></p> <p>Should provide 2 sets (hard copy and soft copy) of:</p> <ol style="list-style-type: none"> 1. User, technical and maintenance manuals should be supplied in English language along with machine diagrams 2. List of equipment and procedures required for local calibration and routine maintenance 3. Service and operation manuals (original and Copy) to be provided 4. Advanced maintenance tasks 	<p><u>DOCUMENTATION</u></p> <p>TO ADD:</p> <ol style="list-style-type: none"> 6. List of essential spares and accessories, with their part number and cost.

	<p>Republic of the Philippines Department of Health, Center for Health Development (CHD) IV-CALABARZON BATANGAS MEDICAL CENTER Batangas City ISO 9001:2015 CERTIFIED</p>	
	 	

documentation	
5. Certificate of calibration and inspection	

H. ITEM 11: 1 UNIT Digital Visual acuity chart

FROM	TO
<p style="text-align: center;"><u>PHYSICAL DESCRIPTION</u></p> <p>Dimensions(metric): Approx. 50*40*21CM (L*W*H)</p>	<p style="text-align: center;"><u>PHYSICAL DESCRIPTION OF THE BOX</u></p> <p><u>Dimensions (metric):</u> (L) 50-60 x (H) 30-40 x (D) 5-25 cm</p>
<p style="text-align: center;"><u>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</u></p> <p>1. Remote control</p>	<p style="text-align: center;"><u>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</u></p> <p>TO ADD: 2. Wall mount bracket (optional)</p>
<p style="text-align: center;"><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p>	<p style="text-align: center;"><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p> <p>Requirements for sign-off: Supplier to perform installation, safety and operation checks before handover. Local clinical staff to affirm completion of installation.</p> <p>Training of staff (medical, technicians): Training of users in operation and basic maintenance shall be provided. Advanced maintenance tasks required shall be documented.</p>
<p style="text-align: center;"><u>WARRANTY</u></p> <p>C. Service Unit: a. In case of Unit Malfunction, Bidder must provide a service unit within 48 hours until such time that the unit has been repaired or replaced.</p>	<p style="text-align: center;"><u>WARRANTY</u></p> <p>C. Service Unit: a. In case of Unit Malfunction, Bidder must provide a service unit within 24-72 hours until such time that the unit has been repaired or replaced.</p>
<p style="text-align: center;"><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine has been in the local or international market for at least five (5) years.</p>	<p style="text-align: center;"><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the hospital equipment/machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that hospital equipment/machine has been in the local or international market for at least five (5) years.</p>





Republic of the Philippines
 Department of Health, Center for Health Development (CHD) IV-CALABARZON
BATANGAS MEDICAL CENTER
 Batangas City
ISO 9001:2015 CERTIFIED



<u>DOCUMENTATION</u>	<u>DOCUMENTATION</u>
<p>Should provide 2 sets (hard copy and soft copy) of:</p> <ol style="list-style-type: none"> 1. User, technical and maintenance manuals should be supplied in English language along with machine diagrams 2. List of equipment and procedures required for local calibration and routine maintenance 3. Service and operation manuals (original and Copy) to be provided 4. Advanced maintenance tasks documentation 5. Certificate of calibration and inspection 	<p>TO ADD:</p> <ol style="list-style-type: none"> 6. List of essential spares and accessories, with their part number and cost.

I. ITEM 12: 1 UNIT Applanation tonometer

<u>FROM</u>	<u>TO</u>
<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Acceptance and Maintenance:</p> <ol style="list-style-type: none"> A. During acceptance: The supplier should conduct actual testing (Qualitative and Quantitative Test) using calibrated analyzers or testing devices. Witnessed by the end users and the technical inspectors. <ol style="list-style-type: none"> a. Valid certificates of the Technicians/Engineers to conduct service/maintenance b. Valid certificates of calibration of the analyzer and testing equipment. c. Provide Service Report per unit d. Calibration Certificates or equivalent e. Acceptance f. Preventive Maintenance Calendar <p>“(NOTE: PROVIDE AND ATTACH DOCUMENT TO PROVE THAT THE ABOVE MENTIONED ARE COMPLIED SUCH as the ff.)”</p> <ol style="list-style-type: none"> a. List of the Engineers/Technicians with their certificates to conduct service and maintenance b. List of the Analyzers/Testing tools with their Brand/Model/Serial No. and its valid certificate of calibration)” c. Sample/Template of Service report and Calibration certificate or equivalent d. Sample/Template of Preventive Maintenance Sticker e. Sample/Template of Preventive Maintenance Calendar 	<p>TO OMIT</p>
<p>Pre- installation requirements: Availability of</p>	<p>TO OMIT</p>

	<p>Republic of the Philippines Department of Health, Center for Health Development (CHD) IV-CALABARZON BATANGAS MEDICAL CENTER Batangas City ISO 9001:2015 CERTIFIED</p>	
---	--	---

<p>5 Amp/15 Amp. Electrical Socket</p> <p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine has been in the local or international market for at least five (5) years.</p>	<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the hospital equipment/machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that hospital equipment/machine has been in the local or international market for at least five (5) years.</p>
--	---

J. ITEM 13: 1 UNIT Trial Lens Set

<u>FROM</u>	<u>TO</u>
<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Acceptance and Maintenance:</p> <p>A. During acceptance: The supplier should conduct actual testing (Qualitative and Quantitative Test) using calibrated analyzers or testing devices. Witnessed by the end users and the technical inspectors.</p> <p>a. Valid certificates of the Technicians/Engineers to conduct service/maintenance</p> <p>b. Valid certificates of calibration of the analyzer and testing equipment.</p> <p>c. Provide Service Report per unit</p> <p>d. Calibration Certificates or equivalent</p> <p>e. Acceptance</p> <p>f. Preventive Maintenance Calendar</p> <p>“(NOTE: PROVIDE AND ATTACH DOCUMENT TO PROVE THAT THE ABOVE MENTIONED ARE COMPLIED SUCH as the ff.)”</p> <p>a. List of the Engineers/Technicians with their certificates to conduct service and maintenance</p> <p>b. List of the Analyzers/Testing tools with their Brand/Model/Serial No. and its valid certificate of calibration)”</p> <p>c. Sample/Template of Service report and Calibration certificate or equivalent</p> <p>d. Sample/Template of Preventive Maintenance Sticker</p> <p>e. Sample/Template of Preventive Maintenance Calendar</p>	<p>TO OMIT</p>



Republic of the Philippines
 Department of Health, Center for Health Development (CHD) IV-CALABARZON
BATANGAS MEDICAL CENTER
 Batangas City
ISO 9001:2015 CERTIFIED



WARRANTY

- A. Warranty Replacement: In case of unit malfunction the bidder should replace the unit with a brand new unit within three months from the start of the warranty period.
 - B. Service and Parts Warranty: at least two (2) years years for both service and parts with quarterly preventive maintenance service
 - C. Service Unit:
 - a. In case of Unit Malfunction, Bidder must provide a service unit within 48 hours until such time that the unit has been repaired or replaced.
 - b. Bidder must have 24/7 readily available Technician to provide technical service and support within 24 hours from report via phone call or email in case of machine breakdown or as needs arise.
 - D. Warranty Certificates: Comprehensive Warranty Certificates, must be included and define in the contract
 - E. Unit, parts, and consumables should be available within 5 years.
- “(NOTE: PROVIDE AND ATTACH SAMPLE/DRAFT FOR THE COMPREHENSIVE WARRANTY CERTIFICATES)”

TO OMIT

DOCUMENTATION

- a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine that the warranty should not be affected with the change of distributor.
In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery
- c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine has been in the local or international market for at least five (5) years.

DOCUMENTATION

- a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the **hospital equipment/machine** that the warranty should not be affected with the change of distributor.
In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery
- c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that **hospital equipment/machine** has been in the local or international market for at least five (5) years

K. ITEM 14: 1 UNIT Prism Set

FROM	TO
<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Acceptance and Maintenance:</p> <ul style="list-style-type: none"> B. During acceptance: The supplier should conduct actual testing (Qualitative and Quantitative Test) using calibrated analyzers or testing devices. Witnessed by the end users and the technical inspectors. 	TO OMIT



Republic of the Philippines
 Department of Health, Center for Health Development (CHD) IV-CALABARZON
BATANGAS MEDICAL CENTER
 Batangas City
ISO 9001:2015 CERTIFIED



<p>a. Valid certificates of the Technicians/Engineers to conduct service/maintenance</p> <p>b. Valid certificates of calibration of the analyzer and testing equipment.</p> <p>c. Provide Service Report per unit</p> <p>d. Calibration Certificates or equivalent</p> <p>e. Acceptance</p> <p>f. Preventive Maintenance Calendar</p> <p>“(NOTE: PROVIDE AND ATTACH DOCUMENT TO PROVE THAT THE ABOVE MENTIONED ARE COMPLIED SUCH as the ff.)”</p> <p>a. List of the Engineers/Technicians with their certificates to conduct service and maintenance</p> <p>b. List of the Analyzers/Testing tools with their Brand/Model/Serial No. and its valid certificate of calibration)”</p> <p>c. Sample/Template of Service report and Calibration certificate or equivalent</p> <p>d. Sample/Template of Preventive Maintenance Sticker</p> <p>e. Sample/Template of Preventive Maintenance Calendar</p>	
<p><u>WARRANTY</u></p> <p>A. Warranty Replacement: In case of unit malfunction the bidder should replace the unit with a brand new unit within three months from the start of the warranty period.</p> <p>B. Service and Parts Warranty: at least two (2) years years for both service and parts with quarterly preventive maintenance service</p> <p>C. Service Unit:</p> <p>a. In case of Unit Malfunction, Bidder must provide a service unit within 48 hours until such time that the unit has been repaired or replaced.</p> <p>b. Bidder must have 24/7 readily available Technician to provide technical service and support within 24 hours from report via phone call or email in case of machine breakdown or as needs arise.</p> <p>D. Warranty Certificates: Comprehensive Warranty Certificates, must be included and define in the contract</p> <p>E. Unit, parts, and consumables should be available within 5 years.</p> <p>“(NOTE: PROVIDE AND ATTACH SAMPLE/DRAFT FOR THE COMPREHENSIVE WARRANTY CERTIFICATES)”</p>	<p>TO OMIT</p>
<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine</p>	<p>TO OMIT</p>






Republic of the Philippines
 Department of Health, Center for Health Development (CHD) IV-CALABARZON
BATANGAS MEDICAL CENTER
 Batangas City
ISO 9001:2015 CERTIFIED



<p>that the warranty should not be affected with the change of distributor.</p> <p>In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>b. Bidder's certificate that the parts shall be available at the authorized Philippine service center/s for a period of 5 years after the warranty period.</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine has been in the local or international market for at least five (5) years.</p> <p>d. For demonstration/confirmation of specification during the evaluation.</p> <p>e. List of essential spares and accessories, with their part number and cost.</p>	
--	--

L. ITEM 15: 1 UNIT Indirect Ophthalmoscope

FROM	TO
<p><u>UTILITY REQUIREMENTS</u></p> <p>Power requirements: 220 to 240V, 50 Hz Battery operated: Internal lithium polymer batteries, rechargeable preferred compatible with both 2.5 V and 3.5 V batteries or handles provided A. Up to 20 hours of ON time with LED illumination.</p>	<p><u>UTILITY REQUIREMENTS</u></p> <p>Power requirements: 220 to 240V, 50 Hz Battery operated: Internal lithium polymer batteries, rechargeable preferred compatible with both 2.5 V and 3.5 V batteries A. Maximum of 20 hours of ON time with LED illumination.</p>
<p><u>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</u></p> <p>2. Charger Input; USB 2.0 Type C: 5V, 1.2 A</p>	<p><u>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</u></p> <p>2. Charger Input: compatible with the machine</p>
<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p>	<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p> <p>Requirements for sign-off: Supplier to perform installation, safety and operation checks before handover. Local clinical staff to affirm completion of installation.</p> <p>Training of staff (medical, technicians): Training of users in operation and basic maintenance shall be provided. Advanced maintenance tasks required shall be documented.</p>
<p><u>WARRANTY</u> C. Service Unit:</p>	<p><u>WARRANTY</u> C. Service Unit:</p>

	<p>Republic of the Philippines Department of Health, Center for Health Development (CHD) IV-CALABARZON BATANGAS MEDICAL CENTER Batangas City ISO 9001:2015 CERTIFIED</p>	 
---	--	---

<p>a. In case of Unit Malfunction, Bidder must provide a service unit within 48 hours until such time that the unit has been repaired or replaced.</p>	<p>a. In case of Unit Malfunction, Bidder must provide a service unit within 24-72 hours until such time that the unit has been repaired or replaced.</p>
<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine has been in the local or international market for at least five (5) years.</p>	<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the hospital equipment/machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that hospital equipment/machine has been in the local or international market for at least five (5) years</p>
<p><u>DOCUMENTATION</u></p> <p>Should provide 2 sets (hard copy and soft copy) of:</p> <ol style="list-style-type: none"> 1. User, technical and maintenance manuals should be supplied in English language along with machine diagrams 2. List of equipment and procedures required for local calibration and routine maintenance 3. Service and operation manuals (original and Copy) to be provided 4. Advanced maintenance tasks documentation 5. Certificate of calibration and inspection 	<p><u>DOCUMENTATION</u></p> <p>TO ADD:</p> <p>6. List of essential spares and accessories, with their part number and cost.</p>
<p><u>SAFETY AND STANDARD</u></p> <ol style="list-style-type: none"> 1. Should be US FDA/CE/BIS/CDSCO approved 2. Manufacturer should have ISO 13485 certification for quality standards. 	<p><u>SAFETY AND STANDARD</u></p> <p>TO ADD:</p> <p>3. ISO 10942:2006 Ophthalmic instruments -- Direct ophthalmoscopes.</p>

M. ITEM 16: 1 UNIT Ophthalmic Ultrasound Scanner

FROM	TO
<p>B-Scan Modes</p> <ol style="list-style-type: none"> 1. Four sets of electronic distance measurement calipers with variable velocity 2. Movie sequence capture up to 20 seconds-real time image viewing and movie editing capability 3. Grey levels: 256 	<p>A-Scan Module Frequency: 10MHz or 11 MHz Electronic Resolution: at least 0.016 mm Immersion or contact measurement mode Time gain control: 0-30 dB Dynamic range: Adjustable from 20 to 110 dB Measurements ACD, lens thickness, VCD,</p>



Republic of the Philippines
 Department of Health, Center for Health Development (CHD) IV-CALABARZON
BATANGAS MEDICAL CENTER
 Batangas City
ISO 9001:2015 CERTIFIED



4. Adjustable gain: 20 to 110 dB
5. Time gain control: 0 to 30 dB
6. Manual and synchronized dynamic adjustment from 25 to 90 dB
7. Unlimited storage capacity for still images and video sequences
8. Image post-processing tools: algorithmic and color images and filters, calipers, areas, angles, markers and comments

Magnetic 10 Mhz Posterior Segment

1. Transducer frequency: 10MHz
2. Axial resolution: at least 150 microns
3. Lateral resolution: at least 300 microns
4. Angle of exploration: at least 50 degrees
5. Depth of exploration: 21 to 60mm
6. Focus: 21 to 25mm

Magnetic 20 Mhz Posterior Segment

1. Transducer frequency: 20MHz
2. Axial resolution: at least 100 microns
3. Lateral resolution: at least 250 microns
4. Angle of exploration: at least 50 degrees
5. Frame rate: up to 16Hz
6. Focus: 24 to 26mm

Magnetic 50 MHz UBM probe with linear scanning for Anterior Segment

1. Transducer frequency: 50 MHz
2. linear transducer movement: exploration width 16mm
3. Focus: 9 to 11mm
4. Axial resolution at least 35 microns
5. Lateral resolution: at least 60 microns

Linear 25 MHz UBM probe

1. Transducer frequency: 25 MHz
2. linear transducer movement: exploration width 16mm
3. Focus: 11 to 13mm
4. Axial resolution at least 70 microns
5. Lateral resolution: at least 120 microns

Standardized A mode

1. Digitally programmed S-shaped amplifier characteristic and comprehensive design criteria for standardized echography and tissue differentiation according to Karl C. Ossining MD
2. Automatic tissue sensitivity determination with specific gain value
3. Diagnosis function: Tumor q1, Retina A1/Retina A2; Musc profile
4. Probe frequency: 8 MHz/parallel beam
5. Depth: orbit 80 microns, eye 40 microns,

axial length

IOL Formulas Hoffer Q, Holladay I, SRK II, SRK/T, Binkhorst II, Haigis, Shammas

B-Scan Module

Frequency: 12 MHz or 15 MHz

Scan Angle: at least 50°

Axial Resolution: at least 0.015 mm

Lateral Resolution: at least 0.040 mm

256 scans per frame

Time gain control: 0-30 dB

Dynamic range: Adjustable from 25 to 90 dB




Image post processing tools: calipers, areas, markers, comment



Republic of the Philippines
 Department of Health, Center for Health Development (CHD) IV-CALABARZON
BATANGAS MEDICAL CENTER
 Batangas City
ISO 9001:2015 CERTIFIED



<p>zoom 20 microns</p> <ol style="list-style-type: none"> 6. Distance measurement between 2 gates with adjustable velocity 7. Axial length measurement with cornea, AC depth, lens and vitreous differentiation <p>System Control Input Devices: USB Keyboard, Mouse & Foot Pedal</p>	
<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p>	<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p> <p>Requirements for sign-off: Supplier to perform installation, safety and operation checks before handover. Local clinical staff to affirm completion of installation.</p> <p>Training of staff (medical, technicians): Training of users in operation and basic maintenance shall be provided. Advanced maintenance tasks required shall be documented.</p>
<p><u>WARRANTY</u></p> <p>C. Service Unit:</p> <ol style="list-style-type: none"> a. In case of Unit Malfunction, Bidder must provide a service unit within 48 hours until such time that the unit has been repaired or replaced. 	<p><u>WARRANTY</u></p> <p>C. Service Unit:</p> <ol style="list-style-type: none"> a. In case of Unit Malfunction, Bidder must provide a service unit within 24-72 hours until such time that the unit has been repaired or replaced.
<p><u>DOCUMENTATION</u></p> <ol style="list-style-type: none"> a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine has been in the local or international market for at least five (5) years. 	<p><u>DOCUMENTATION</u></p> <ol style="list-style-type: none"> a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the hospital equipment/machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that hospital equipment/machine has been in the local or international market for at least five (5) years
<p><u>DOCUMENTATION</u></p> <p>Should provide 2 sets (hard copy and soft copy) of:</p> <ol style="list-style-type: none"> 1. User, technical and maintenance manuals should be supplied in English language along with machine diagrams 2. List of equipment and procedures required for local calibration and routine 	<p><u>DOCUMENTATION</u></p> <p>TO ADD:</p> <ol style="list-style-type: none"> 6. List of essential spares and accessories, with their part number and cost.

	Republic of the Philippines Department of Health, Center for Health Development (CHD) IV-CALABARZON BATANGAS MEDICAL CENTER Batangas City ISO 9001:2015 CERTIFIED	 
---	---	--

maintenance 3. Service and operation manuals (original and Copy) to be provided 4. Advanced maintenance tasks documentation 5. Certificate of calibration and inspection	
---	--

N. ITEM 17: 1 UNIT Lasers, Nd:YAG, Ophthalmic



FROM	TO
YAG Mode Laser source: Q-switched Nd-YAG Wavelength shall be 1,064 nm Pulse width shall be 3ns Burst mode shall be 1, 2 and 3 pulses per trigger Cone angle at least 16 degrees Pulse repetition rate: at least 3 HZ (single)/1.5 Hz (burst) Output energy: 0.3 to 10.0 mL/pulse Spot size: 8um Focus shift: 0 to +/- 500 um Aiming beam: 635nm LED Slit lamp illumination Magnification shall be $\leq 25x$ ii. Working distance shall be 100 mm DISPLAYS/CONTROLS i. Selected energy is required ii. Shot selection is required iii. Power output is required iv. Shot counter is required	YAG Mode Laser source: Q-switched Nd-YAG or Super Gaussian Beam Profile Wavelength shall be 1,064 nm Pulse width shall be 3-4ns Burst mode shall be 1, 2 and 3 pulses per trigger Cone angle at least 16 degrees Pulse repetition rate: at least 2.5-3 HZ (single)/1.5 Hz (burst) or double & Triple total of 1.5Hz Output energy: 0.3 to 10.0 mL/pulse Spot size: 8-10 um Focus shift: 0 to +/- 500 um Aiming beam: 635-650 nm Slit lamp illumination: LED or Halogen Magnification shall be $\leq 25x$ with or without 38x magnification ii. Working distance shall be more or less at 100 mm DISPLAYS/CONTROLS i. Selected energy is required ii. Shot selection is required iii. Power output is required iv. Shot counter is required
<u>PHYSICAL DESCRIPTION</u> Dimensions: approx 13.6in Wx 16.6 in Dx 22.7 in H	<u>PHYSICAL DESCRIPTION</u> System Dimensions: 125 – 670mm(W) x 250 – 430mm (D) x 65 – 730mm(H)
<u>UTILITY REQUIREMENTS</u> Power requirements: 200-230 VAC 50/60 Hz\	<u>UTILITY REQUIREMENTS</u> Power requirements: 100-240V/200-230VAC, 50/60 Hz
<u>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</u>	<u>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</u>



Republic of the Philippines
 Department of Health, Center for Health Development (CHD) IV-CALABARZON
BATANGAS MEDICAL CENTER
 Batangas City
ISO 9001:2015 CERTIFIED



Spare bulb - 3V DC 3-4W	Spare bulb compatible with the machine provided
<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p>	<p><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p> <p>Requirements for sign-off: Supplier to perform installation, safety and operation checks before handover. Local clinical staff to affirm completion of installation.</p> <p>Training of staff (medical, technicians): Training of users in operation and basic maintenance shall be provided. Advanced maintenance tasks required shall be documented.</p>
<p><u>WARRANTY</u></p> <p>C. Service Unit:</p> <ol style="list-style-type: none"> a. In case of Unit Malfunction, Bidder must provide a service unit within 48 hours until such time that the unit has been repaired or replaced. 	<p><u>WARRANTY</u></p> <p>C. Service Unit:</p> <ol style="list-style-type: none"> a. In case of Unit Malfunction, Bidder must provide a service unit within 24-72 hours until such time that the unit has been repaired or replaced.
<p><u>DOCUMENTATION</u></p> <ol style="list-style-type: none"> a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine has been in the local or international market for at least five (5) years. 	<p><u>DOCUMENTATION</u></p> <ol style="list-style-type: none"> a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the hospital equipment/machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that hospital equipment/machine has been in the local or international market for at least five (5) years
<p><u>DOCUMENTATION</u></p> <p>Should provide 2 sets (hard copy and soft copy) of:</p> <ol style="list-style-type: none"> 1. User, technical and maintenance manuals should be supplied in English language along with machine diagrams 2. List of equipment and procedures required for local calibration and routine maintenance 3. Service and operation manuals (original and Copy) to be provided 	<p><u>DOCUMENTATION</u></p> <p>TO ADD:</p> <ol style="list-style-type: none"> 6. List of essential spares and accessories, with their part number and cost.

	<p>Republic of the Philippines Department of Health, Center for Health Development (CHD) IV-CALABARZON BATANGAS MEDICAL CENTER Batangas City ISO 9001:2015 CERTIFIED</p>	
---	--	---




4. Advanced maintenance tasks documentation 5. Certificate of calibration and inspection	
---	--

O. ITEM 18: 1 UNIT Refracting Chair

FROM	TO
<p><u>TECHNICAL DESCRIPTION</u></p> <p>The Ophthalmic chair's height is adjustable. Easy operation by foot control switch.</p> <p>Up & down stroke: 120mm Load lifting: maximum 200kg</p>	<p><u>TECHNICAL DESCRIPTION</u></p> <p>The Ophthalmic chair's height is adjustable. Easy operation by foot control switch or any remote control device that is compatible for controls.</p> <p>Up & down stroke: 120-150mm Load lifting: maximum 250kg</p>
<p><u>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</u></p> <p>1. 1Lamp with LED bulb Wattage: 24V, 7W</p>	<p><u>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</u></p> <p>TO ADD: 2. Table: 850×450mm (optional)</p>
<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine has been in the local or international market for at least five (5) years.</p>	<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the hospital equipment/machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that hospital equipment/machine has been in the local or international market for at least five (5) years</p>

P. ITEM 19: 1 UNIT Operating Table

FROM	TO
<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine</p>	<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the hospital equipment/machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that hospital</p>

	<p>Republic of the Philippines Department of Health, Center for Health Development (CHD) IV-CALABARZON BATANGAS MEDICAL CENTER Batangas City ISO 9001:2015 CERTIFIED</p>	 
---	--	---





has been in the local or international market for at least five (5) years.	equipment/machine has been in the local or international market for at least five (5) years
--	--

Q. ITEM 20: 1 UNIT Operating Room (Surgeon’s) Chair

TO OMIT FROM THE LIST OF MEDICAL EQUIPMENT FOR PUBLIC BIDDING

R. ITEM 21: 1 UNIT Plasma Sterilizer

FROM	TO
<p style="text-align: center;"><u>UTILITY REQUIREMENTS</u></p> <p>Power consumption: 60-90W</p> <p style="text-align: center;"><u>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</u></p> <ol style="list-style-type: none"> 1. External thermal printer 2. Cart with locking wheel Dimensions: at least 603mmx660mmx483mm Wheel type: steel with high grade plastic cover 	<p style="text-align: center;"><u>UTILITY REQUIREMENTS</u></p> <p>Power consumption: Max. Power 1kVA</p> <p style="text-align: center;"><u>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</u></p> <p>TO ADD:</p> <ol style="list-style-type: none"> 3. Rotary sealer 4. Compatible sterile packaging pouch made from high density polyethylene fiber material that is safe for hydrogen peroxide sterilization, with the following sizes: (100mm wide x 400mm long) (200mm wide x 400mm long) (300mm wide x 400mm long) 5. Hydrogen Peroxide Cassette – good for at least 30 cycles 6. Vacuum sealed pouch that can be stored up to 6 months in sealed sterile condition, with the following sizes: (135mm wide x 280mm long) (240mm wide x 410mm long) 7. Chemical indicator tape – for sterilization cycle monitor
<p style="text-align: center;"><u>ENVIRONMENTAL REQUIREMENTS</u></p> <p>Storage condition: Capable of being stored continuously in ambient temperature of 0 to 40 deg C and relative humidity of 15 to 90%</p>	<p style="text-align: center;"><u>ENVIRONMENTAL REQUIREMENTS</u></p> <p>Storage condition: Temperature: 10-40°C Humidity: 30-85%</p>
<p style="text-align: center;"><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p>	<p style="text-align: center;"><u>TRAINING, INSTALLATION & UTILIZATION</u></p> <p>Pre- installation requirements: Availability of 5 Amp/15 Amp. Electrical Socket</p> <p>Requirements for sign-off: Supplier to perform installation, safety and operation checks before handover. Local clinical staff to affirm completion of installation.</p>

	Republic of the Philippines Department of Health, Center for Health Development (CHD) IV-CALABARZON BATANGAS MEDICAL CENTER Batangas City ISO 9001:2015 CERTIFIED	
		

	Training of staff (medical, technicians): Training of users in operation and basic maintenance shall be provided. Advanced maintenance tasks required shall be documented.
<p><u>WARRANTY</u></p> <p>C. Service Unit:</p> <p>a. In case of Unit Malfunction, Bidder must provide a service unit within 48 hours until such time that the unit has been repaired or replaced.</p>	<p><u>WARRANTY</u></p> <p>C. Service Unit:</p> <p>a. In case of Unit Malfunction, Bidder must provide a service unit within 24-72 hours until such time that the unit has been repaired or replaced.</p>
<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the anesthesia machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that anesthesia machine has been in the local or international market for at least five (5) years.</p>	<p><u>DOCUMENTATION</u></p> <p>a. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin of the hospital equipment/machine that the warranty should not be affected with the change of distributor. In case said Certification is not available in time of Opening of Bids, Bidder must submit it during delivery</p> <p>c. Certification from the manufacturer authenticated by the Philippine Consulate from the country of origin that hospital equipment/machine has been in the local or international market for at least five (5) years</p>

S. Item22: Telescopic Laryngoscopy

FROM	TO
<p><u>DELIVERY</u></p> <p>30 to 60 days from the receipt of Purchase Order.</p>	<p><u>DELIVERY</u></p> <p>30 to 90 days from the receipt of Purchase Order.</p>

This Supplemental / Bid Bulletin shall form part of the Bidding Documents. Any provisions in the Bidding Documents inconsistent herewith is hereby amended, modified and superseded accordingly.

For guidance and information of all concerned.

(Sgd.) ELIZABETH V. PALINES, MD, FPPS, FCNSP, FPNA
 Chairperson, HBAC

Received by the bidder:

 Signature over printed name

Date Received: _____