



HOSPITAL BIDS AND AWARDS COMMITTEE
 SUPPLEMENTAL BID BULLETIN NO. 1
IB 2021-002
 PRE-BID CONFERENCE (MARCH 09, 2021)

I. GENERAL INSTRUCTIONS

- Bidders are required to submit one (1) soft copy of the original documents clearly scanned in multiple pages in one (1) PDF File per the three required files to the designated Google Form link.
- Documentary requirements on the electronic bidding is the same as in the manual bidding as provided in the 2016 Revised Implementing Rules and Regulations (IRR) of Republic Act 9184 (RA 9184), otherwise known as the “Government Procurement Reform Act” and Resolution No. 09-2020 of the Government Procurement Policy Board entitled “Approving Measures for the Efficient Conduct of Procurement Activities During a State of Calamity, or Implementation of Community Quarantine or Similar Restrictions”
- The BAC is using the 6th Edition of the Philippine Bidding Documents and all Amendments Forms therein.
- Due to limited slots in Zoom, only one (1) representative per bidder will be allowed to enter.
- Bidder shall only provide the password of their encrypted file upon being called and acknowledged in the Online Bidding Conference by the BAC before the opening of said Bidder’s bid documents. Bidder’s video should be on during this process.
- For the issuance of the Official Receipt, bidders may get the same at the Cash Collection Section or Procurement Section, during office hours, M-F; 8:00AM-5:00PM, except holidays, and upon showing of proof of payment. For the purpose of the bidding, those who submitted the proof of payment early will be verified by our Cash Collection Section and will be provided a soft copy of the Official Receipt, otherwise, other proof of payment will be acceptable subject to later verification by the Cash Collection Section.
- The winning bidder is required to produce two (2) hard copies of the scanned document anytime before the award. The same can be personally sent or via courier. Any discrepancy on the submitted soft copy as bidder during the bidding conference and hard copies as winning bidder is a ground for disqualification.
- The scanned copy should have the required original signature. E-signature is not allowed.
- Bidder must have completed, within the period specified in the Invitation to Bid, an SLCC that is similar to the contract to be bid, and whose value, adjusted to current prices using the Philippine Statistics Authority (PSA) consumer price indices, must be at least fifty percent (50%) of the ABC. However, in the case of Expendable Supplies, said SLCC must be at least twenty five percent (25%) of the ABC. Service will fall on the Expendable Supplies.
- If there is no single completed contract for the required amount, the bidder may submit at least two (2) completed similar contracts and the aggregate contract amounts should be equivalent to at least the percentage of the ABC as required above and the largest of these similar contracts must be equivalent to at least half of the percentage of the ABC as required.
- A contract shall only be considered “similar” to the contract to be bid if it is of similar nature.
- Contracts similar to the Project should be completed within two (2) years to the deadline for the submission and receipt of bids.

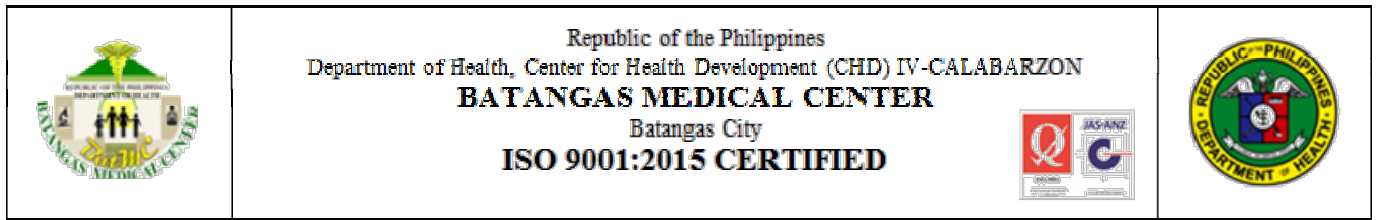

- Bidders must submit updated Tax clearance per E.O. No. 398, s. 2005, as finally reviewed and approved by the Bureau of Internal Revenue (BIR).
- Bidders are required to provide physical demonstration of the equipment being offered a day after the bid opening. This requirement may be replaced with referral to other institution with same equipment were the TWG and End Users may conduct physical or virtual demo provided the bidder will certify the impossibility of providing actual demo due to justifiable circumstances. Should there be a certification, it is understood that should the equipment offered but was not demonstrated be delivered and later inspected to be not in compliance with the required equipment as stated in the bid, the procuring entity reserves its right to reject acceptance of the delivered equipment in addition to any other penalty that can be imposed against the bidder.
- Bidders will only need to submit one eligibility documents for all equipment comprising the project: Supply and Delivery of Various Medical Equipment for COVID-19 Response IB2021-002. They are required to accomplish the technical specification for each equipment they wish to participate as reflected in the bid document.
- Indicate the brand and packing of items offered
- The brand offered should be commercially available on the market for at least five (5) years. Certification to be submitted
- Swapping/replacement of equivalent drugs/supplies will not be tolerated and will be considered as a violation. Swapping/replacement of items shall be grounds for blacklisting. REASON: The Technical Working Group has evaluated the bid product. If the items will be swapped with another equivalent brand, thus no proper conduct of evaluation was made for the swapped product, putting BatMC at risk.
- Bidders shall submit Notarized certificate of Exclusive Distributorship between/ or Authority to Distribute from the manufacturer or principal Distributor
- All winning bidders shall submit a certificate of commitment to deliver the products awarded to them
- It is understood that the Contractor is legally responsible to deliver all issued purchase order/s and failure to deliver the first Purchase Order as scheduled shall mean automatic cancellation of the PO and Notice of Award (NOA). Upon cancellation, the BAC shall proceed to qualify the second lowest bidder if applicable; or proceed to Negotiated Procurement. The Winning Contractor who failed to deliver shall shoulder the price difference (from the second lowest bidder) of the item in addition to the acquired liquidated damages.
- Bidders must specify in the Technical Specifications Form under Bidder's Offer, Technical Specifications Column the exact specifications they are offering and must indicate the reference page number in the user manual submitted against each of the individual parameters. Whereas, bidders must state either "Comply" or "Not Comply" under the Bidder's Offer, Statement of Compliance Column. The bids with incomplete and incorrect filled out Technical Specifications Form will be disqualified.
- Please take note of the delivery period as this will be strictly implemented due to the effectivity period of the budget. Should the item be delivered late with the budget having lapsed, the contract will be automatically terminated.

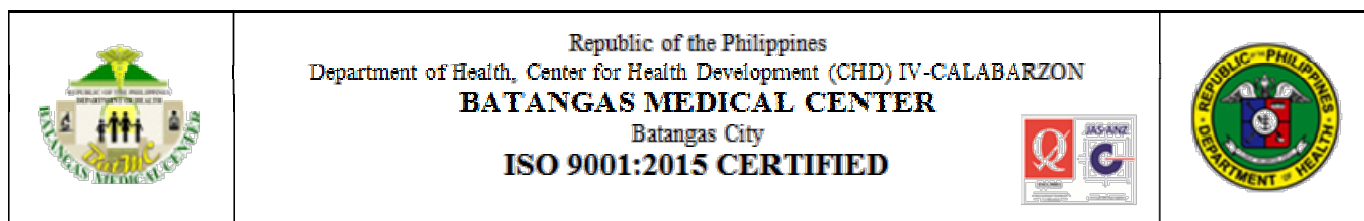

II. Amendment of Terms of Specifications / Terms of Reference as per the Pre-Bidding Conference conducted last March 09, 2021 are as follows:

IB 2021-002A SUPPLY AND DELIVERY OF 4 UNIT SYRINGE PUMP



FROM	TO
<p>DIMENSIONS: 300 mm (W) x 100 mm (H) x 90 mm (D) to 381 mm (W) x 120 mm (H) x 112 mm (D) Weight: 1.5 - 2.5 kg Large format LCD/TFT display</p>	<p>DIMENSIONS: 300 mm (W) x 100 mm (H) x 90 mm (D) to 381 mm (W) x 120 mm (H) x 180 mm (D) Weight: 1.5 - 2.5 kg Large format LCD/TFT display</p>

IB 2021-002B SUPPLY AND DELIVERY OF 3 UNIT VOLUMETRIC INFUSION PUMP

FROM	TO
<p>PHYSICAL DESCRIPTION 253 mm (W) x 120 mm (H) x 102 mm (D) to 120 mm (W) x 200 mm (H) x 142 mm (D) approx. 1.5kg to 3 kg Compatible disposables: dedicated infusion sets (with Free Flow Protection)</p>	<p>PHYSICAL DESCRIPTION 250-385mm (W) x 120-200mm (H) x 100-140mm (D) approx. 1.5kg to 3 kg Compatible disposables: universal or open system infusion sets (with Free Flow Protection)</p>

IB 2021-002C SUPPLY AND DELIVERY OF 1 UNIT DEFIBRILLATOR

FROM	TO
<p>PRINTER:</p> <ul style="list-style-type: none"> - manual, automatic (10"pre and post recording) - integrated thermal printer for ECG traces and events documentation including HR/SpO2/NIBP values - paper speed: 5, 10, 25, 50 mm/sec. - paper width: 58 mm 	<p>PRINTER:</p> <ul style="list-style-type: none"> - manual, automatic (10"pre and post recording) - integrated thermal printer for ECG traces and events documentation including HR/SpO2/NIBP values - paper speed: 5-50 mm/sec. - paper width: 50-80 mm
<p>PHYSICAL DESCRIPTION:</p> <ul style="list-style-type: none"> - high contrast TFT colour LCD 5.7" (320x240 pixel) to LCD 7" (800x480 dots) - ECG through the discharge paddles (1 trace) or through 5, 10 leads patient cable for 3, 6, or 12 traces and SpO2 value Automatic change over when plugging the patient cable - filters: 50/60 Hz, base line, EMG - heart rate indicator - Weight: 5.5 kg to 6.5 kg with battery 	<p>PHYSICAL DESCRIPTION:</p> <ul style="list-style-type: none"> - high contrast TFT colour LCD 5.7" (320x240 pixel) to LCD 7" (800x480 dots) - ECG through the discharge paddles (1 trace) or through 5, 3-5 leads patient cable for 3, 6, or 12 traces and SpO2 value Automatic change over when plugging the patient cable - filters: 50/60 Hz, base line, EMG - heart rate indicator - Weight: 5.5 kg to 6.5 kg with battery
<p>UTILITY REQUIREMENT:</p> <ul style="list-style-type: none"> - Internal rechargeable battery (charging time 	<p>UTILITY REQUIREMENT:</p> <ul style="list-style-type: none"> - Internal rechargeable battery (Lithium ion

	<p>Republic of the Philippines Department of Health, Center for Health Development (CHD) IV-CALABARZON BATANGAS MEDICAL CENTER Batangas City ISO 9001:2015 CERTIFIED</p>	
---	--	---



<p>95%: 2 hours) AC 220V-240 VAC, 60 Hz - Memory: internal flash at least 4 GB or up to 300 hours of ECG data, events and usage review</p>	<p>battery), charging time 95%: 2 hours, AC 220V-240 VAC, 60 Hz - Memory: internal flash at least 4 GB or up to 300 hours of ECG data, events and usage review</p>
<p>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</p> <ul style="list-style-type: none"> - Cable with banana plugs, IEC - Limb clamp set of 4 - Chest bulb set of 6 - Glasgow algorithm* in GB, IT, DE - 1 roll paper - Rechargeable battery 	<p>ACCESSORIES, CONSUMABLES, SPARE PARTS, OTHER COMPONENT</p> <ul style="list-style-type: none"> - Cable with banana plugs, IEC - Limb clamp set of 4 - Disposable electrodes - 1 roll paper - Rechargeable battery - Glasgow algorithm in GB, IT, DE (optional)
<p>DELIVERY SCHEDULE:</p> <ul style="list-style-type: none"> - 30 days upon receipt of P.O 	<ul style="list-style-type: none"> - To retain

IB 2021-002D SUPPLY AND DELIVERY OF 1 UNIT ECG PEDIATRIC

FROM	TO
<p>PHYSICAL DESCRIPTION:</p> <ul style="list-style-type: none"> - Compact lightweight design with carrying handles - USB port for data transmission and external printer connection - Dimensions <ul style="list-style-type: none"> • 190mm x 120mm x 60mm to 410mm x 316x 136mm Weight • 1kg to 4kg 	<p>PHYSICAL DESCRIPTION:</p> <ul style="list-style-type: none"> - Compact lightweight design with carrying handles or provision of cart if no handles - USB port for data transmission and external printer connection - Dimensions <ul style="list-style-type: none"> • 190mm x 120mm x 30mm to 410mm x 316x 136mm Weight • 1kg to 6kg
<p>UTILITY REQUIREMENT:</p> <p>Electrical Battery <ul style="list-style-type: none"> • Lithium ion Battery recharge <ul style="list-style-type: none"> • Four hours per battery to full capacity Main power <ul style="list-style-type: none"> • 100-240VAC, 50/60Hz Power consumption <ul style="list-style-type: none"> • 60W max </p>	<p>UTILITY REQUIREMENT:</p> <p>Electrical Battery <ul style="list-style-type: none"> • Lithium ion Battery recharge <ul style="list-style-type: none"> • Four hours per battery to full capacity Main power <ul style="list-style-type: none"> • 220-240VAC, 60Hz Power consumption <ul style="list-style-type: none"> • 60W max </p>

IB 2021-002E SUPPLY AND DELIVERY OF ECG MACHINE (ADULT)

FROM	TO
<p>TECHNICAL DESCRIPTION:</p> <p>Display Size - At least 8.5 inches</p> <p>Resolution</p>	<p>TECHNICAL DESCRIPTION:</p> <p>Display Size - 7 – 8.5 inches</p> <p>Resolution</p>

	<p>Republic of the Philippines Department of Health, Center for Health Development (CHD) IV-CALABARZON BATANGAS MEDICAL CENTER Batangas City ISO 9001:2015 CERTIFIED</p>	
---	--	---

<p>- 320 x 240 LCD or higher</p> <p>UTILITY REQUIREMENT:</p> <p>Electrical</p> <p>Battery</p> <ul style="list-style-type: none"> • Lithium ion <p>Battery recharge</p> <ul style="list-style-type: none"> • Four hours per battery to full capacity <p>Main power</p> <ul style="list-style-type: none"> • 100-240VAC, 50/60Hz <p>Power consumption</p> <ul style="list-style-type: none"> • 60W max <p>DELIVERY SCHEDULE:</p> <p>- 30 calendar days from receipt of P.O</p>	<ul style="list-style-type: none"> • 320 x 240 LCD or higher <p>UTILITY REQUIREMENT:</p> <p>Electrical</p> <p>Battery</p> <ul style="list-style-type: none"> • Lithium ion <p>Battery recharge</p> <ul style="list-style-type: none"> • Four hours per battery to full capacity <p>Main power</p> <ul style="list-style-type: none"> • 220-240VAC, 60Hz <p>Power consumption</p> <ul style="list-style-type: none"> • 60W max <p>- To retain</p>
---	---

IB 2021-002F SUPPLY AND DELIVERY OF 3 UNIT CARDIAC MONITOR - PEDIATRIC

FROM	TO
<p>TECHNICAL DESCRIPTION:</p> <p>Parameter: HR, BP, Spo2, RR, PR, EtCo2, ECG</p> <p>Network: Connected to central monitoring System by hardwire/wireless</p> <p>Alarm: high and low limits alarm Audible and visual alarm Software update through networking port or USB port</p> <p>Indicator: Dual alarm indicator lights Power indicator light Battery indicator light</p>	<p>TECHNICAL DESCRIPTION:</p> <p>Parameter: HR, BP, Spo2, RR, PR, EtCo2 (can be side stream or mainstream as long as the price will remain within the ABC), ECG</p> <p>Network: Connected to central monitoring System by hardwire/wireless. Provision of Central Monitoring System (optional)</p> <p>Alarm: high and low limits alarm Audible and visual alarm Software update through networking port or USB port</p> <p>Indicator: Dual alarm indicator lights Power indicator light Battery indicator light</p>
<p>PHYSICAL DESCRIPTION:</p> <p>Display: 5-10 inches TFT touch screen Net Weight 2 to 4kg with carrying handle Resolution: 800x600 or higher</p>	<p>PHYSICAL DESCRIPTION:</p> <p>Display: 5-15 inches TFT touch screen Net Weight 2 to 4kg with carrying handle Resolution: 800x600 or higher</p>
<p>UTILITY REQUIREMENT:</p> <p>AC100-240V 6a/3a 50/60Hz, 150VA Battery: built in and rechargeable lithium ion Operating time: 3 hours</p>	<p>UTILITY REQUIREMENT:</p> <p>AC220-240V, 60Hz Battery: built in and rechargeable lithium ion Operating time: 2-4 hours</p>



Republic of the Philippines
 Department of Health, Center for Health Development (CHD) IV-CALABARZON
BATANGAS MEDICAL CENTER
 Batangas City
ISO 9001:2015 CERTIFIED



IB 2021-002I SUPPLY AND DELIVERY OF DRY FOG HYDROGEN PEROXIDE STERILIZER

FROM	TO
<p><u>TECHNICAL DESCRIPTION:</u></p> <p>Remote Control</p>	<p><u>TECHNICAL DESCRIPTION:</u></p> <p>To Retain</p>
	<p>To add:</p> <p><u>TECHNICAL DESCRIPTION:</u> With 90-120 second delay in fogging: This delay, further limits the potential for inappropriate exposure to the hydrogen peroxide solution.</p>
<p><u>PHYSICAL DESCRIPTION:</u></p> <p>700mm*700mm*560mm</p>	<p><u>PHYSICAL DESCRIPTION:</u></p> <ul style="list-style-type: none"> - With Handle - Timer Dial - Disinfectant Fluid Level Indicator - With 2-4 pcs caster 3-5 inches wheels with breaks or available cart for easy maneuver - L: 12 – 20 inches - W: 12 – 20 inches - H : 20 - 35 inches - Can disinfect an area of at least 36 square meters to 75 square meters with a ceiling height of 3 meters.
	<p>To add:</p> <p><u>CONSUMABLES:</u> Hydrogen Peroxide dry fogging solution</p> <ul style="list-style-type: none"> - Disinfectant fogging solution that contains Hydrogen Peroxide 3-7% and with or without 0.005% - 0.1 mg/L Elemental Silver - FDA certified and included in the US Environmental Protection Agency (EPA) N list as a disinfecting and sterilizing agent via fogging and has been used successfully in a number of hospitals - Clear, pale coloured liquid. Non flammable and will not support combustion - Hydrogen Peroxide dry fogging solution 500-600L - Provision of operation chart, indicate Time, Volume and Area
<p><u>TRAINING, INSTALLATION & UTILIZATION:</u></p> <ul style="list-style-type: none"> - Safety and operation check before 	<p><u>TRAINING, INSTALLATION & UTILIZATION:</u></p> <ul style="list-style-type: none"> - Safety and operation check before handover



Republic of the Philippines
 Department of Health, Center for Health Development (CHD) IV-CALABARZON
BATANGAS MEDICAL CENTER
 Batangas City
ISO 9001:2015 CERTIFIED



<p>handover</p> <ul style="list-style-type: none"> - End user’s training in operation - Basic maintenance and user care 	<ul style="list-style-type: none"> - Basic maintenance and user care - Persons charged with the handling and cleaning of the product must be trained prior to start their work and in regular intervals. They must be informed about the risks using the product and the measures to take for efficient prevention. This concerns particularly working security, first aid, and health and environment protection. - Must provide a material safety data sheet for the disinfectant solution that contains information on the potential hazards (health, fire, reactivity and environmental) and how to work safely with the chemical product. - Demo and return demo for end users
	<p>CERTIFICATIONS:</p> <ul style="list-style-type: none"> - Provide Certificate of Product Registration (CPR) or its equivalent document for the Hydrogen Peroxide dry fogging solution - Provide LTO or any Certification to operate and sell the product provided by the Philippine Government such as FDA for the Dry Fog Hydrogen Peroxide Sterilizer Machine

(Sgd.) ELIZABETH V. PALINES, MD, FPPS, FCNSP, FPNA
 Chairperson, HBAC

Received by the bidder:

 Signature over printed name
 Date Received: _____